Knight®
by Midmark

Midmark Corporation • P O Box 286 • 60 Vista Drive
Versailles • Ohio • 45380-0286 • www.midmark.com
Phone: 937-526-3662 Fax: 937-526-5542

Optional Tray Installation for Asepsis 21 Unit

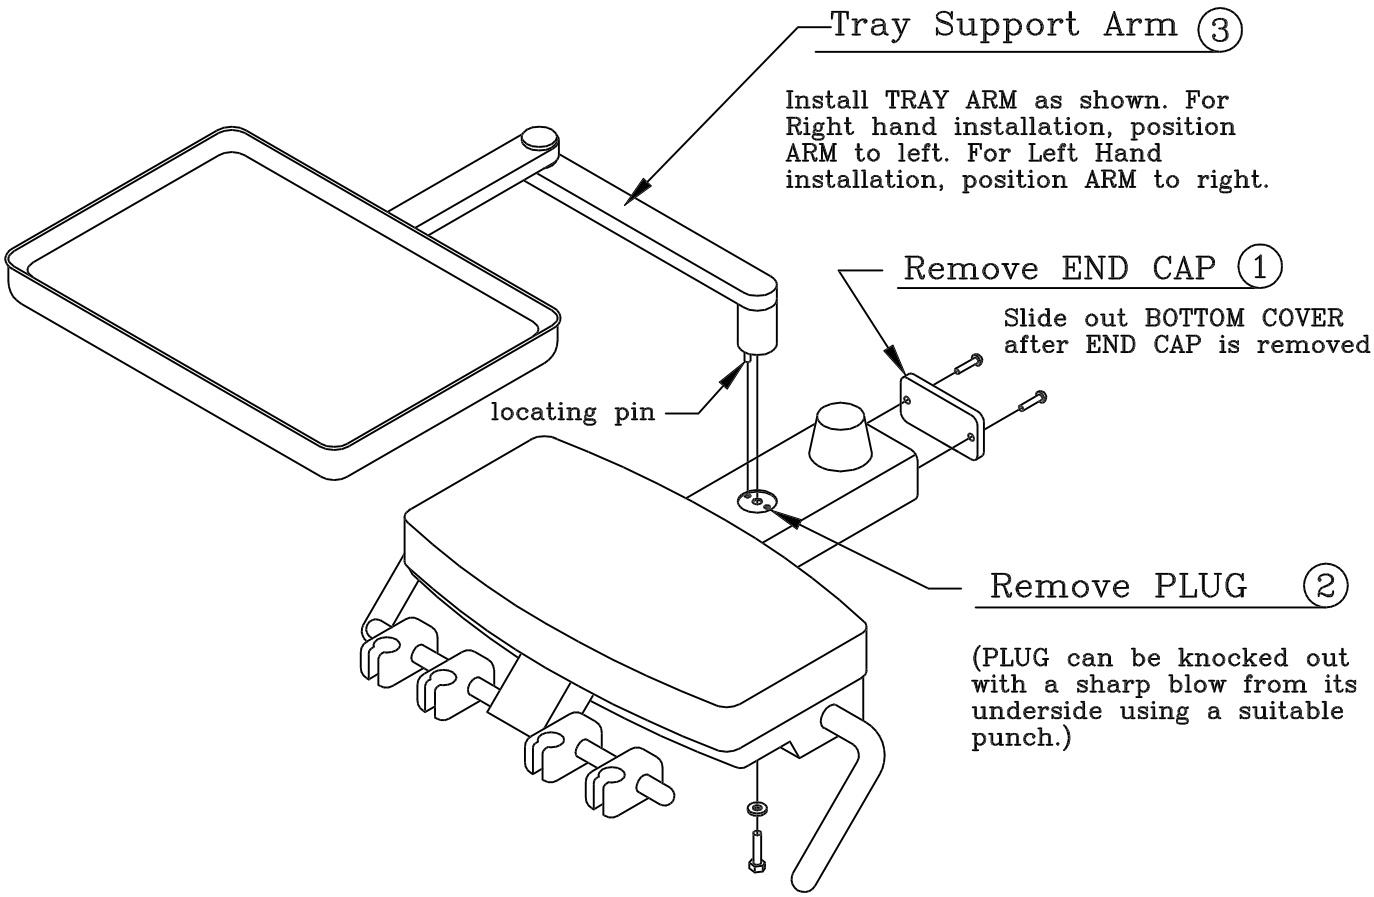
Tray Support Arm (3)
Install TRAY ARM as shown. For Right hand installation, position ARM to left. For Left Hand installation, position ARM to right.
Remove END CAP (1)
Slide out BOTTOM COVER after END CAP is removed
locating pin
Remove PLUG (2)
(PLUG can be knocked out with a sharp blow from its underside using a suitable punch.)